



—7.266

3.711  
3.685  
3.676  
3.650  
3.461  
3.439  
3.419  
2.115  
2.012  
1.660  
1.644  
1.441  
1.430  
1.312  
1.290  
0.901  
0.885  
0.868  
-0.000

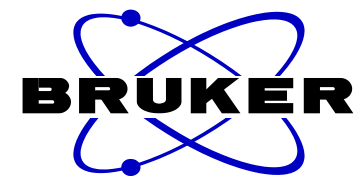

NAME 149822  
EXPNO 1  
PROCNO 1  
Date\_ 20210605  
Time\_ 17.48 h  
INSTRUM Avance  
PROBHD Z116098\_0833 (  
PULPROG zg30  
TD 65536  
SOLVENT CDCl3  
NS 16  
DS 2  
SWH 8196.722 Hz  
FIDRES 0.250144 Hz  
AQ 3.9977460 sec  
RG 101  
DW 61.000 usec  
DE 13.54 usec  
TE 293.9 K  
D1 1.00000000 sec  
TD0 1  
SFO1 400.1324708 MHz  
NUC1 1H  
P0 3.33 usec  
P1 10.00 usec  
SI 65536  
SF 400.1300073 MHz  
WDW EM  
SSB 0  
LB 0.30 Hz  
GB 0  
PC 1.00

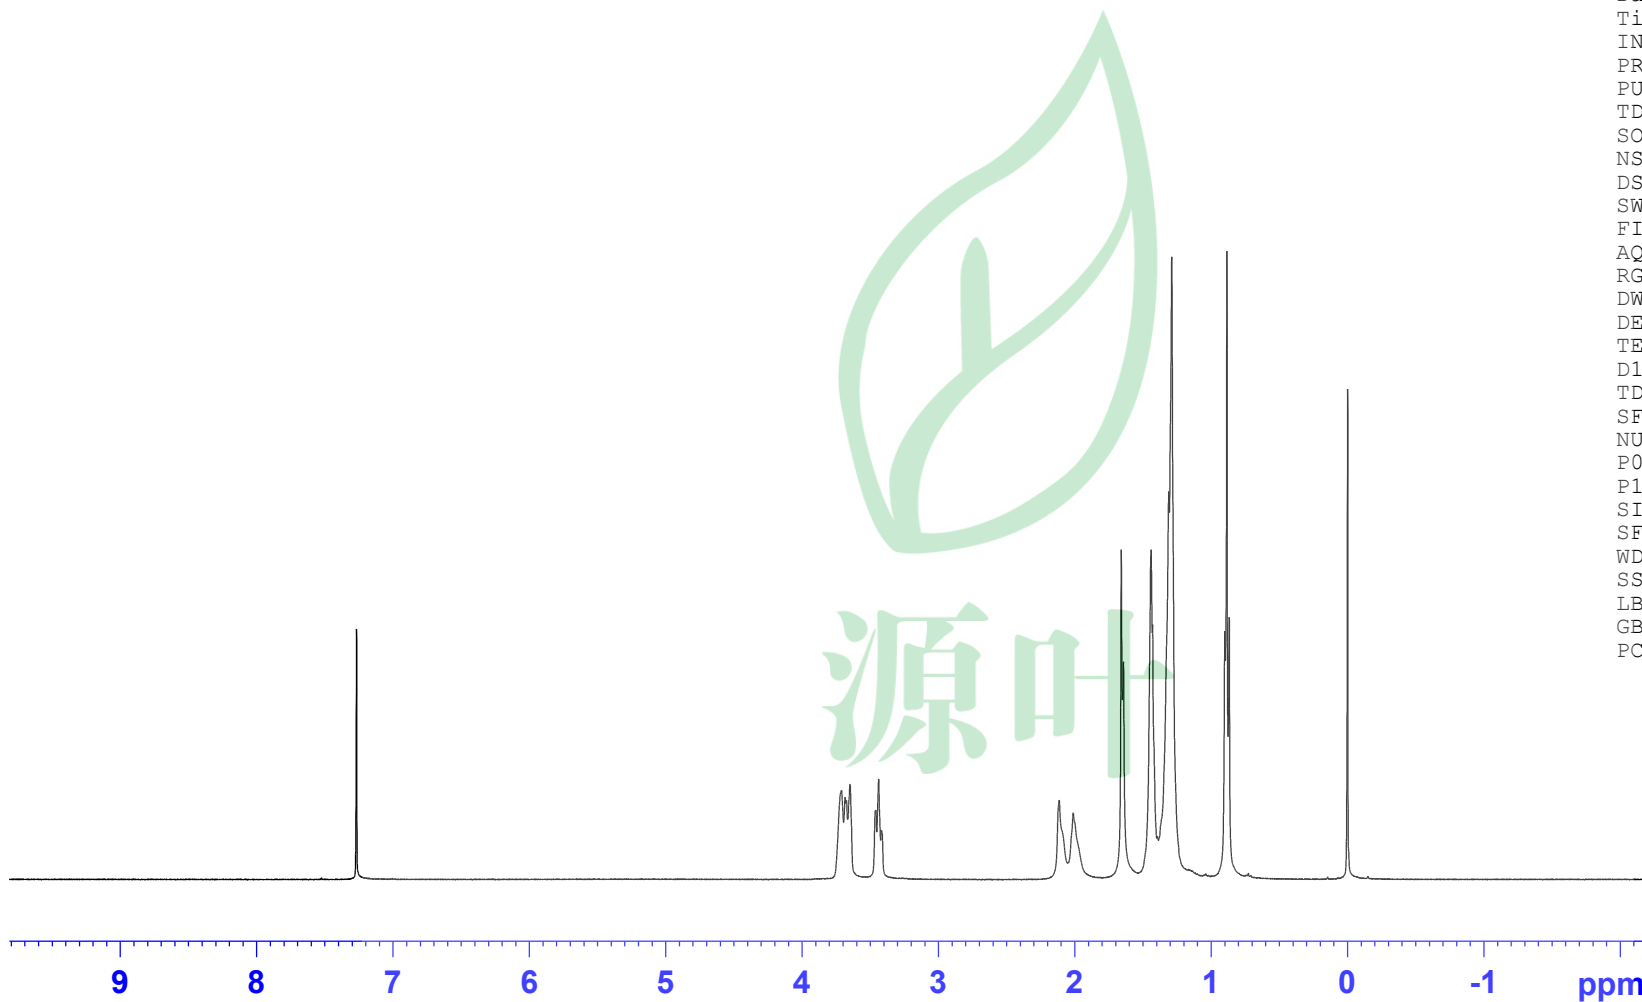

1.96  
1.00  
1.92  
1.99  
3.06  
7.17  
3.03