

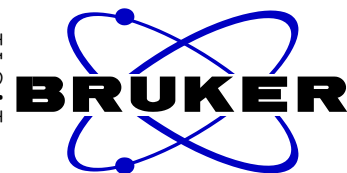


—7.268

2.382
2.363
2.344
2.212
2.205
2.195
2.188
2.177
2.170
1.952
1.946
1.939
1.690
1.672
1.653
1.634
1.615
1.558
1.539
1.521
1.504
1.470
1.453
1.443
1.435
1.431
1.425
1.421
1.413
1.397
1.379
1.363
1.351
1.345
1.341

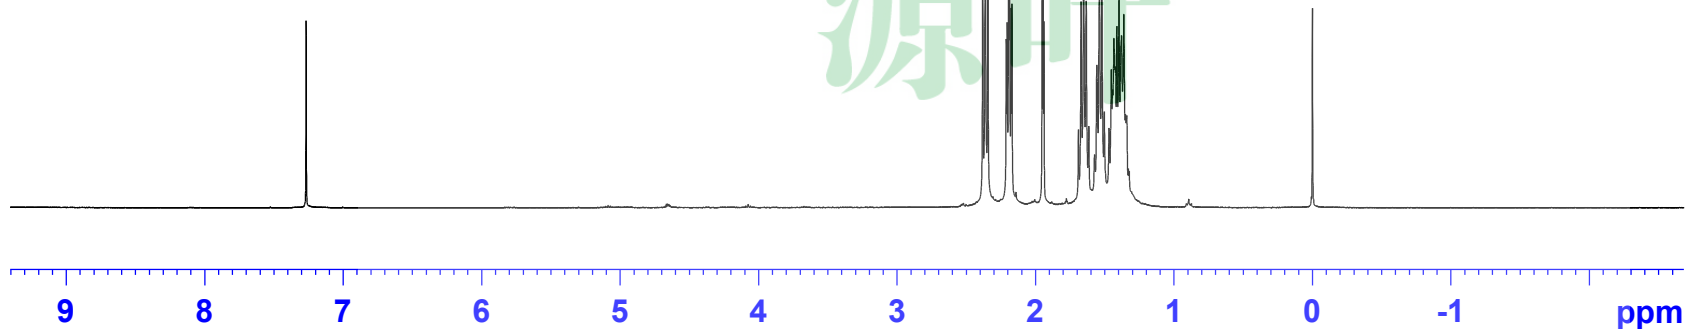

NAME 150801
EXPNO 1
PROCNO 1
Date_ 20210613
Time_ 14.07 h
INSTRUM Avance
PROBHD Z116098_0833 (
PULPROG zg30
TD 65536
SOLVENT CDCl3
NS 16
DS 2
SWH 8196.722 Hz
FIDRES 0.250144 Hz
AQ 3.9977460 sec
RG 101
DW 61.000 usec
DE 13.54 usec
TE 294.4 K
D1 1.00000000 sec
TD0 1
SFO1 400.1324708 MHz
NUC1 1H
P0 3.33 usec
P1 10.00 usec
SI 65536
SF 400.1300064 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

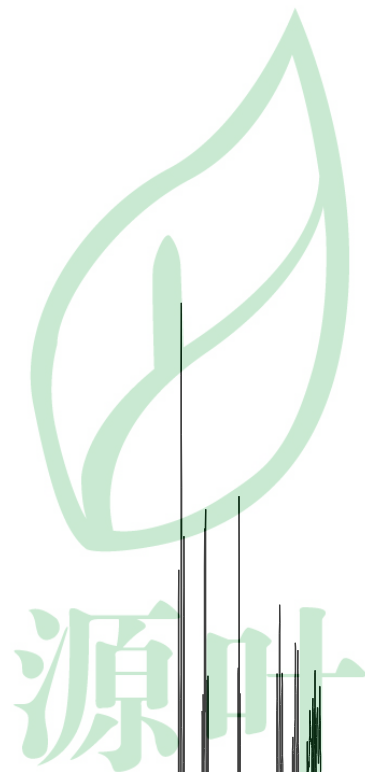

2.33
2.26
1.00
2.47
2.47
4.85