
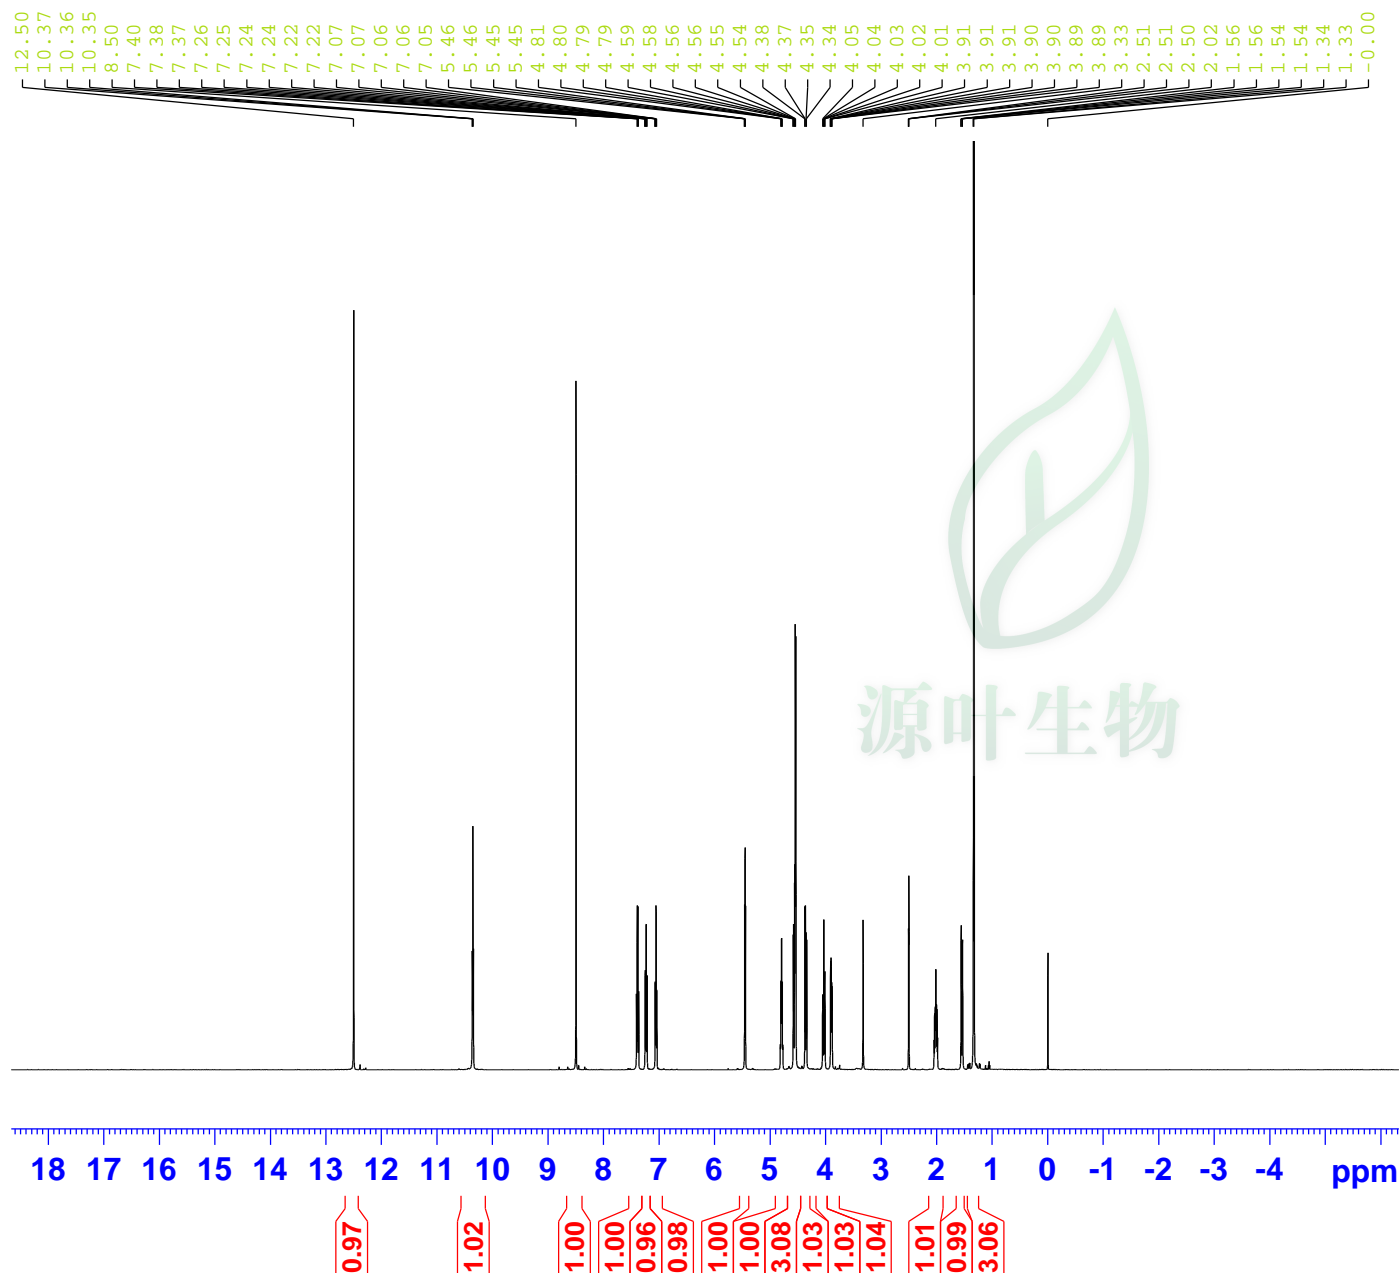


DLTW-419-S-DMSO-150612

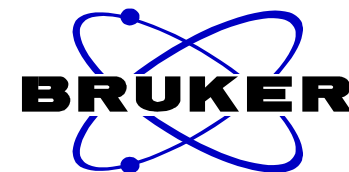

Current Data Parameters

NAME DLTW-419-S-DMSO-150612
EXPNO 1
PROCNO 1

F2 - Acquisition Parameters

Date_ 20150612
Time 15.34
INSTRUM spect
PROBHD 5 mm PABBO BB/
PULPROG zg30
TD 74998
SOLVENT DMSO
NS 8
DS 2
SWH 15000.000 Hz
FIDRES 0.200005 Hz
AQ 2.4999332 sec
RG 60.69
DW 33.333 usec
DE 6.50 usec
TE 298.1 K
D1 1.00000000 sec
TD0 1

===== CHANNEL f1 =====

SFO1 600.1337060 MHz
NUC1 1H
P1 10.50 usec
PLW1 23.00000000 W

F2 - Processing parameters

SI 65536
SF 600.1300018 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00