


MASS SPECTROMETRY REPORT

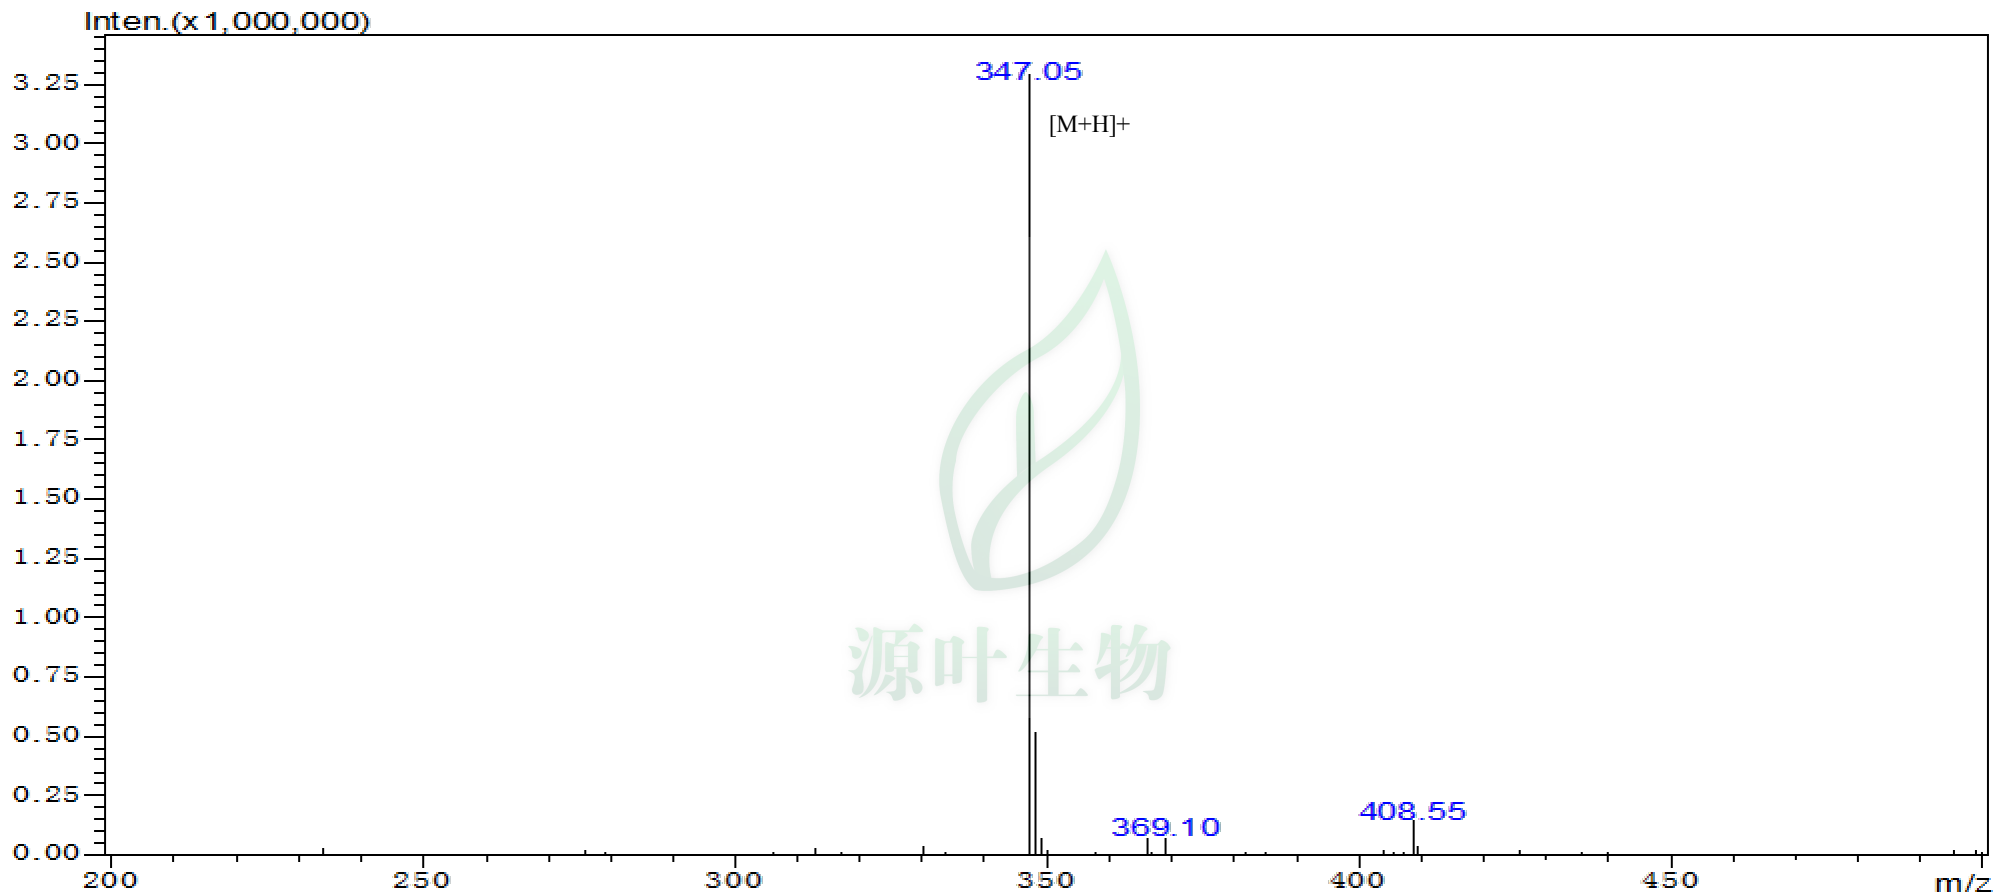

Sample Description		Instrument		SHIMADZU LCMS-2010EV	
Analyzed date:	2016-11-28	Probe:	ESI	Probe Bias:	+4.5kv
Analyst:	Long	Nebulizer Gas Flow:	1.5L/min	Detector:	1.5kv
Sample:	RGD RD-3	CDL:	-20.0v	T. Flow:	0.2ml/min
M.W.:	346.35	CDL Temp.:	250 °C	B. Conc.:	50%H2O/50%ACN
Lot. No.:	P161128-LL187565	Block Temp.:	200 °C		