


Date Acquired: 2019/5/28 15:19:50
Tray# : 1
Vial#: 4
Injection Volume: 1
Processed by: Admin

Peak#1 Ret.Time:Averaged 5.583-5.600(Scan#:671-673)
BG Mode:Calc 5.458<->5.842(656<->702)
Mass Peaks:7 Base Peak:884.95(108225) Polarity:Neg Segment1 - Event1

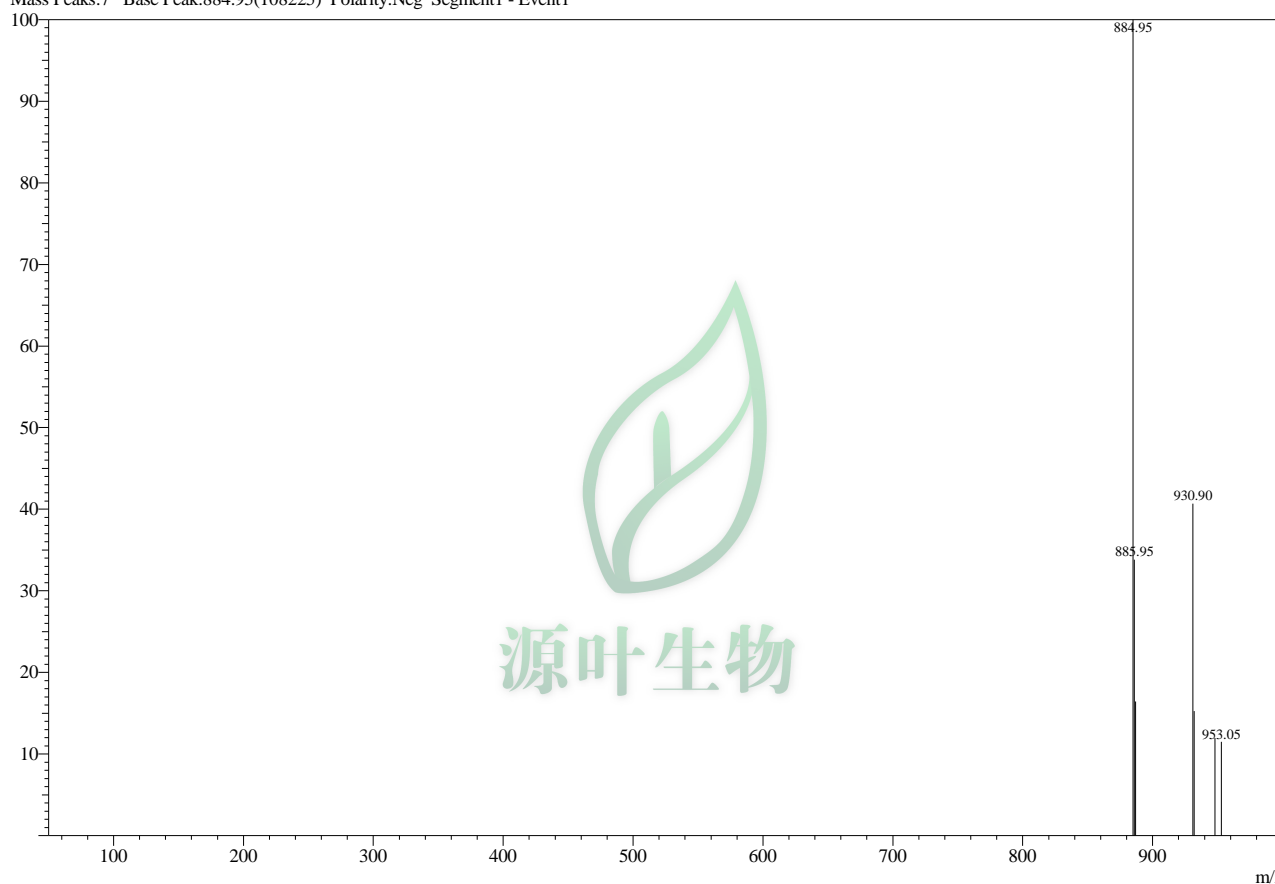

MS Spectrum Table

Peak#:1 Ret.Time:
BG Mode:Calc 5.458<->5.842(656<->702)
Mass Peaks:7 Base Peak:884.95(108225) Polarity:Neg Segment1 - Event1

#	m/z	Abs.Inten.	Rel.Inten.	Charge	Polarity	Monoisotopic
1	884.95	108225	100.00			
2	885.95	36598	33.82			
3	887.00	17773	16.42			
4	930.90	44015	40.67			