


7.288  
7.267  
7.261  
7.185  
7.164  
— 6.463

4.662  
4.648  
4.634  
2.981  
2.963  
2.945  
2.898  
2.856  
2.838  
2.817  
2.805  
2.787  
1.772  
1.757  
1.708  
1.691  
1.601  
1.584  
1.567  
1.294  
1.284  
1.270  
1.202

NAME	S82442
EXPNO	4000
PROCNO	1
Date_	20200313
Time_	20.30 h
INSTRUM	Avance
PROBHD	5 mm
PULPROG	zg30
TD	65536
SOLVENT	CDCl3
NS	8
DS	0
SWH	8620.689 Hz
FIDRES	0.263083 Hz
AQ	3.8011379 sec
RG	101
DW	58.000 usec
DE	12.49 usec
TE	300.0 K
D1	1.00000000 sec
TD0	1
SFO1	400.1819009 MHz
NUC1	1H
P1	9.56 usec
SI	65536
SF	400.1800090 MHz
WDW	EM
SSB	0
LB	0.30 Hz
GB	0
PC	1.00

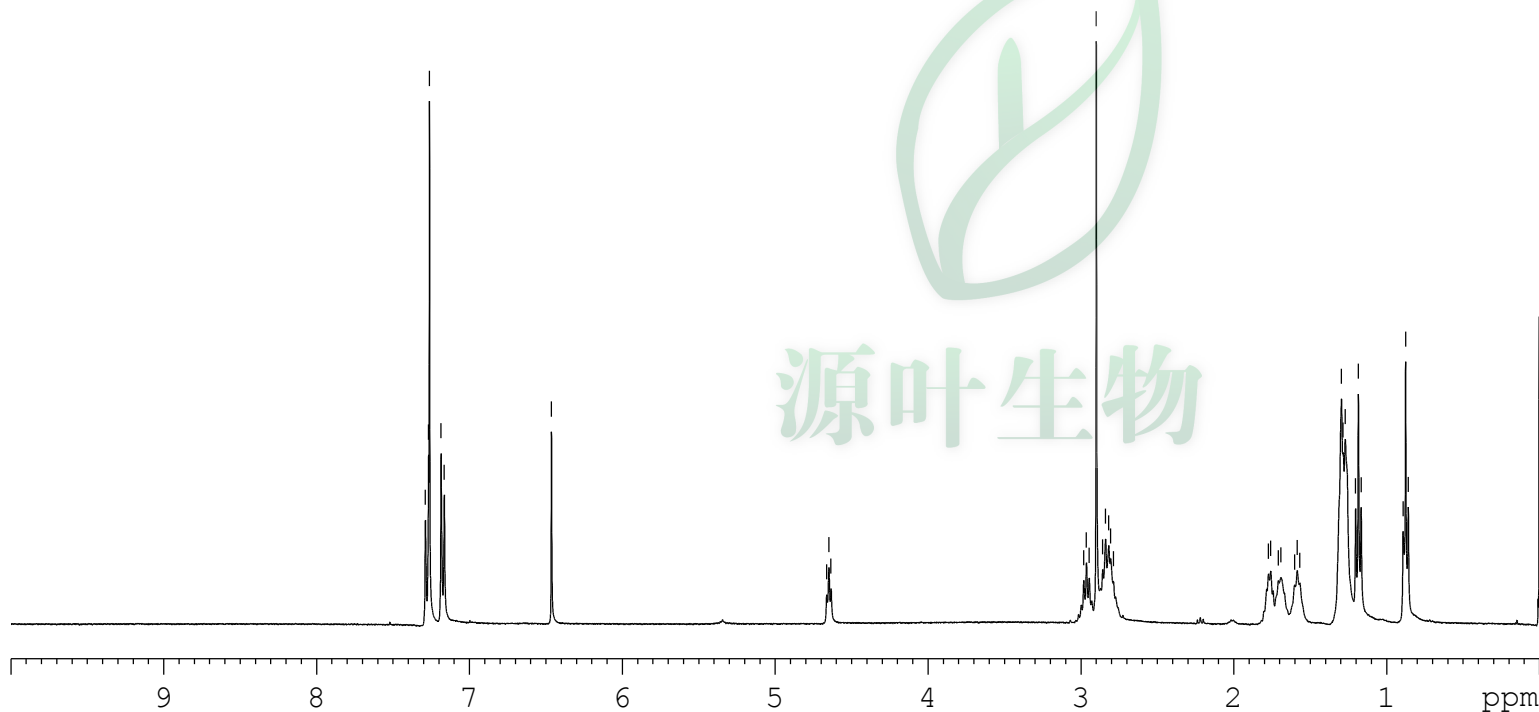

2.38  
1.90

0.79

0.93

1.53  
3.00  
3.71

1.51  
1.78  
1.95  
8.04  
3.36  
3.12