


NAME 114103
EXPNO 400
PROCNO 1
Date_ 20200617
Time 18.11
INSTRUM spect
PROBHD 5 mm 5MM

PULPROG zg30
TD 65536
SOLVENT DMSO
NS 8
DS 0
SWH 8620.689 Hz
FIDRES 0.131541 Hz
AQ 3.8011379 sec
RG 203
DW 58.000 usec
DE 6.50 usec
TE 300.0 K
D1 1.00000000 sec
TD0 1

===== CHANNEL f1 =====
NUC1 1H
P1 13.22 usec
PL1 -3.00 dB
PL1W 20.99974442 W
SFO1 400.1319006 MHz
SI 32768
SF 400.1300060 MHz
WDW EM
SSB 0
LB 0.30 Hz
GB 0
PC 1.00

7.627
7.539
7.518
7.406
7.386

3.336
2.691
2.672
2.654
2.635
2.512
2.508
2.504
2.499
2.495
1.911
1.229
1.215
1.196
1.177

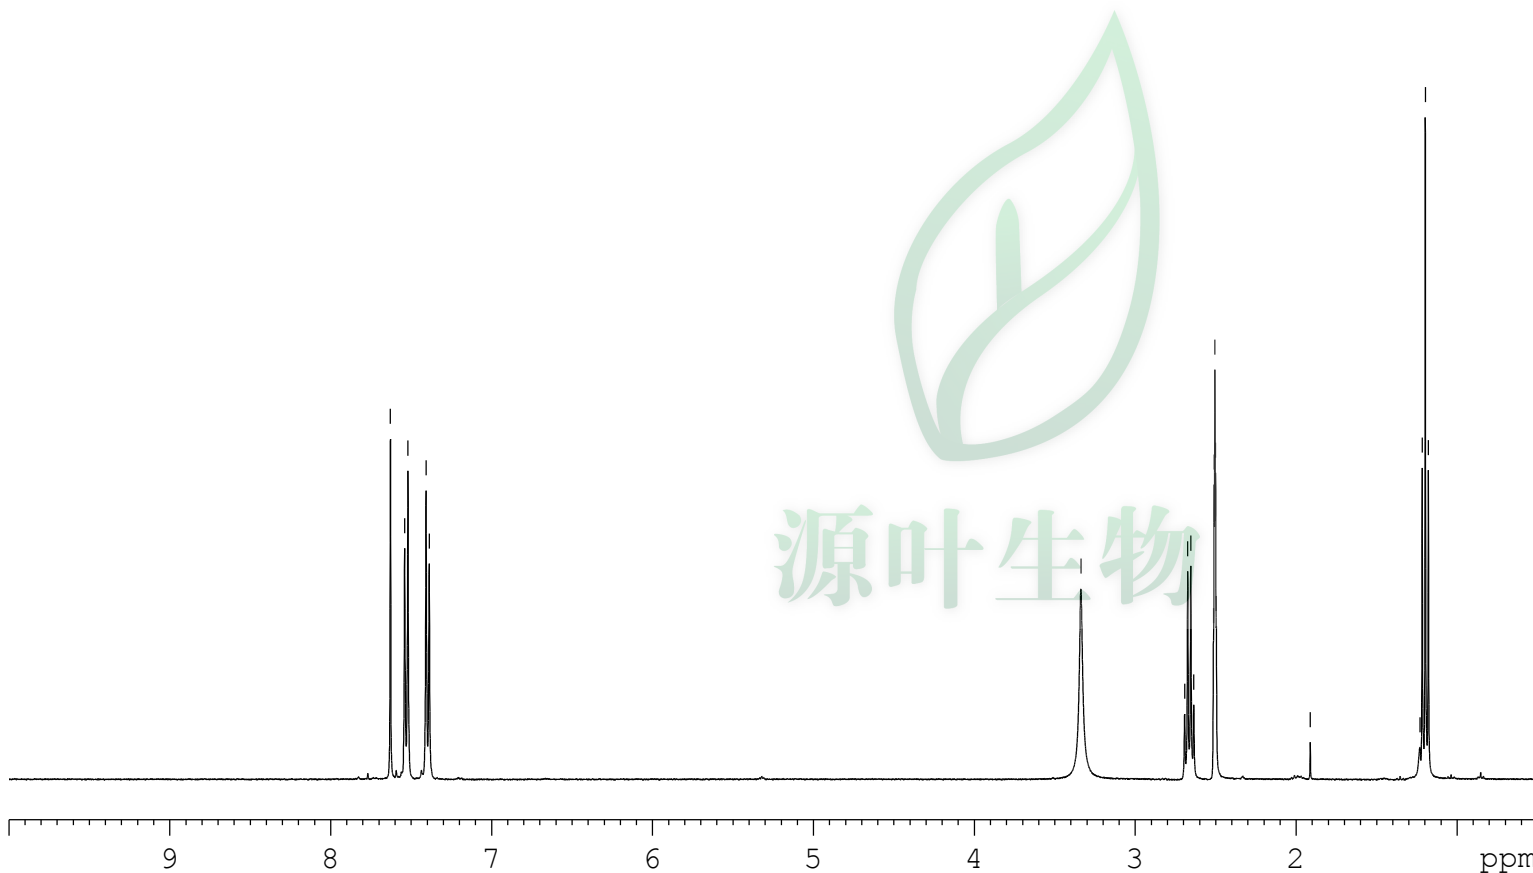

1.20
2.40
2.41

2.41

4.02